

FIG. 1



FIG. 1

FIG. 2



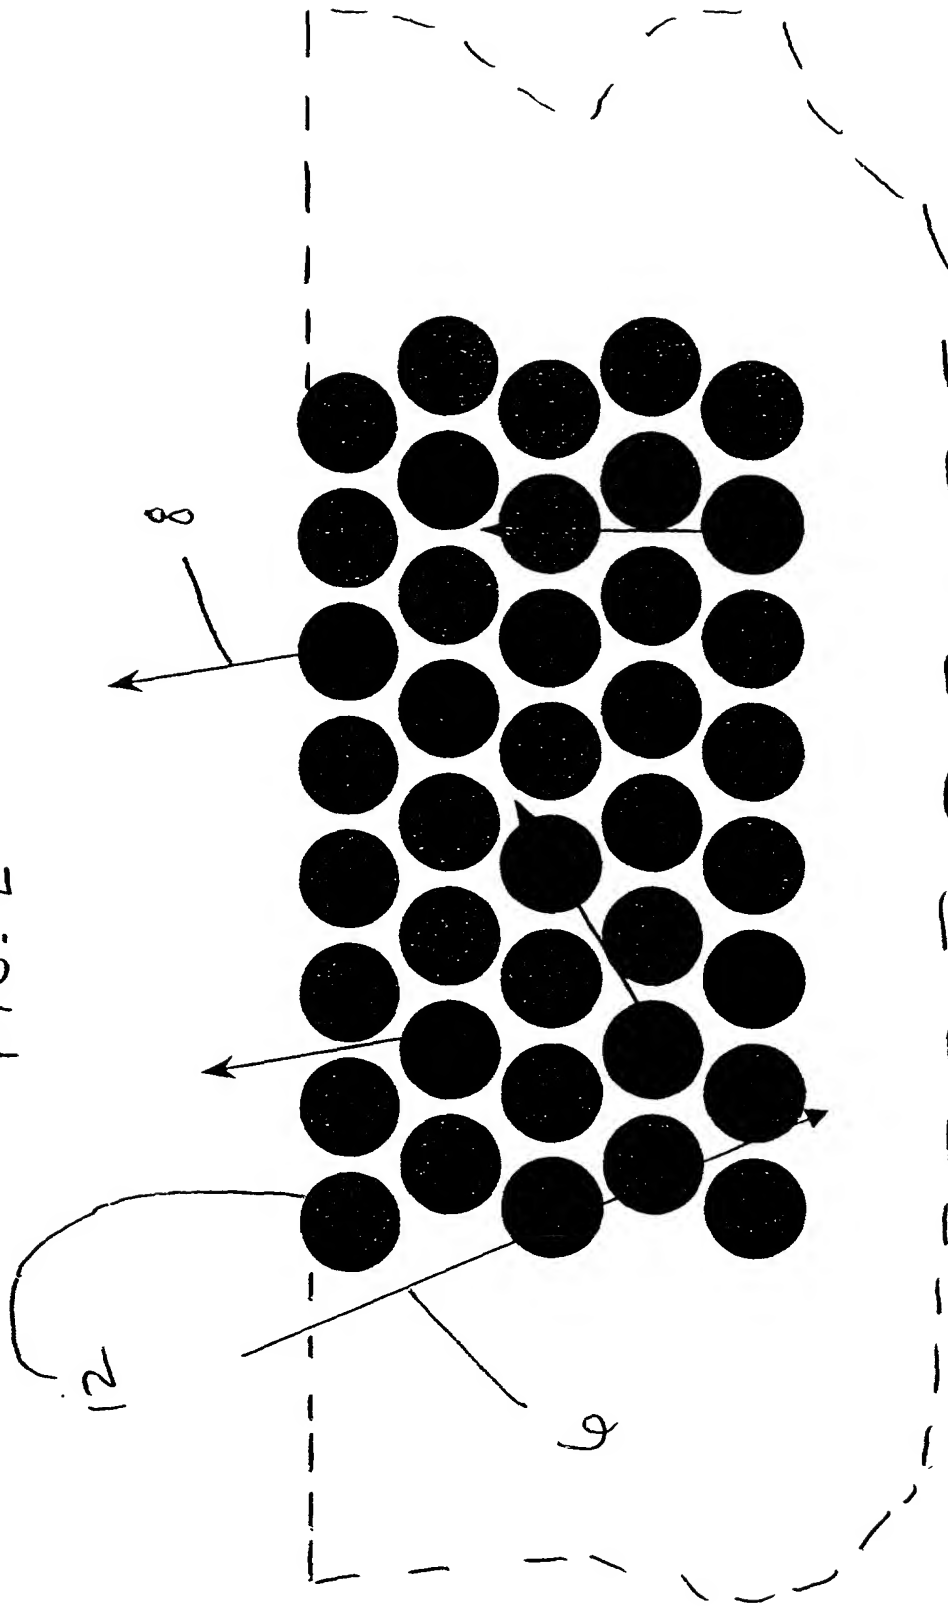


FIG. 3

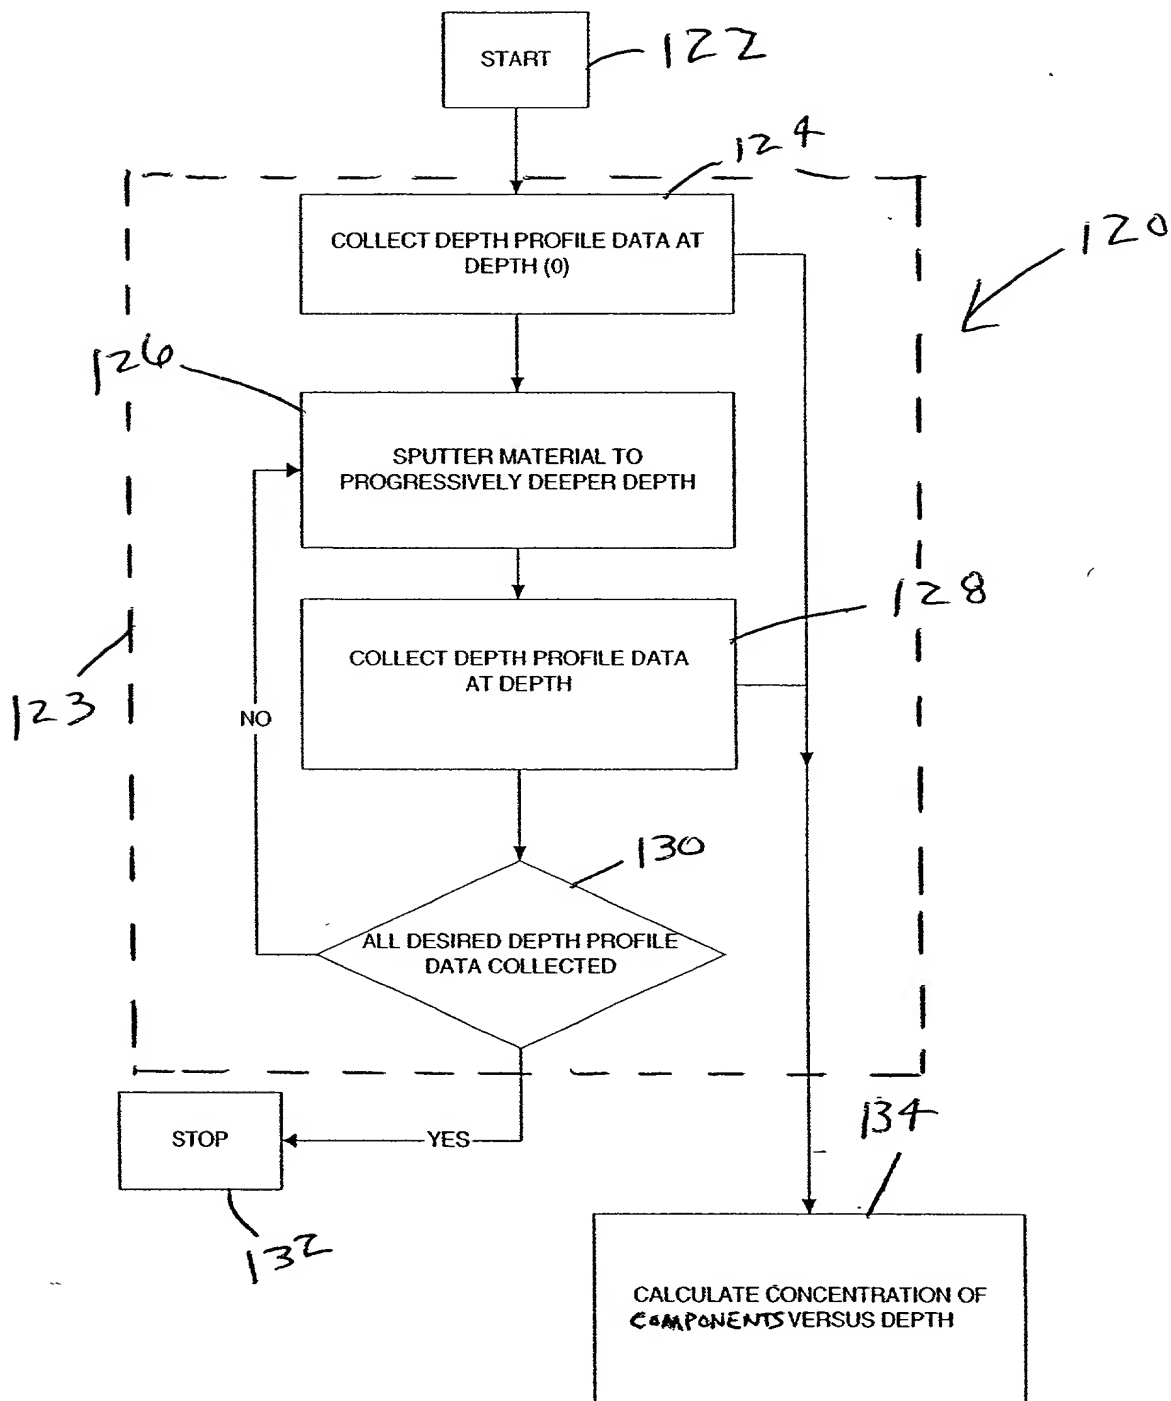

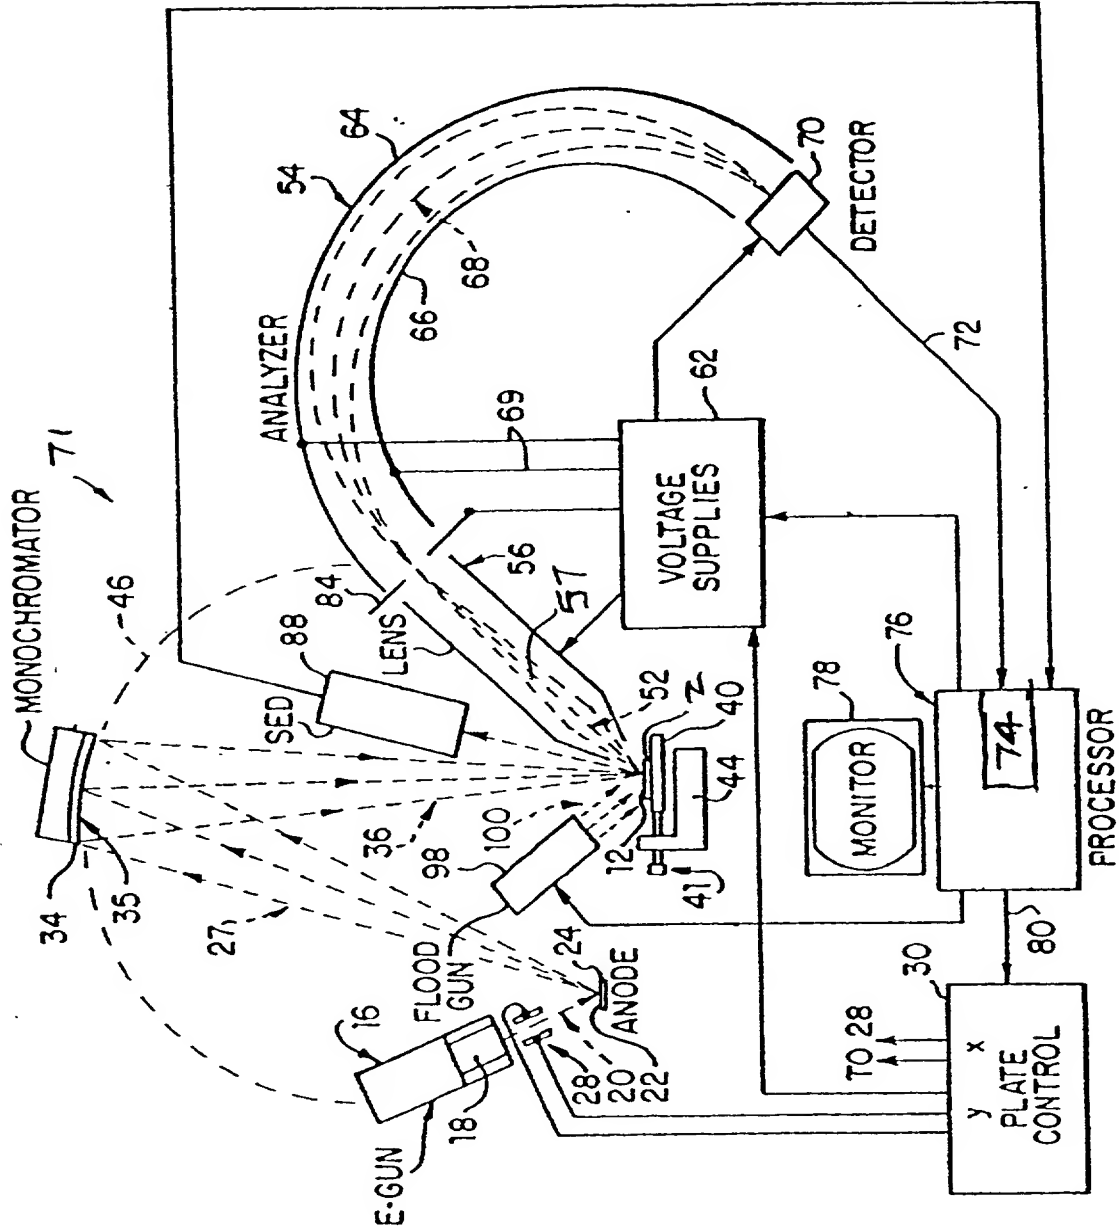

SCANNED, # _____

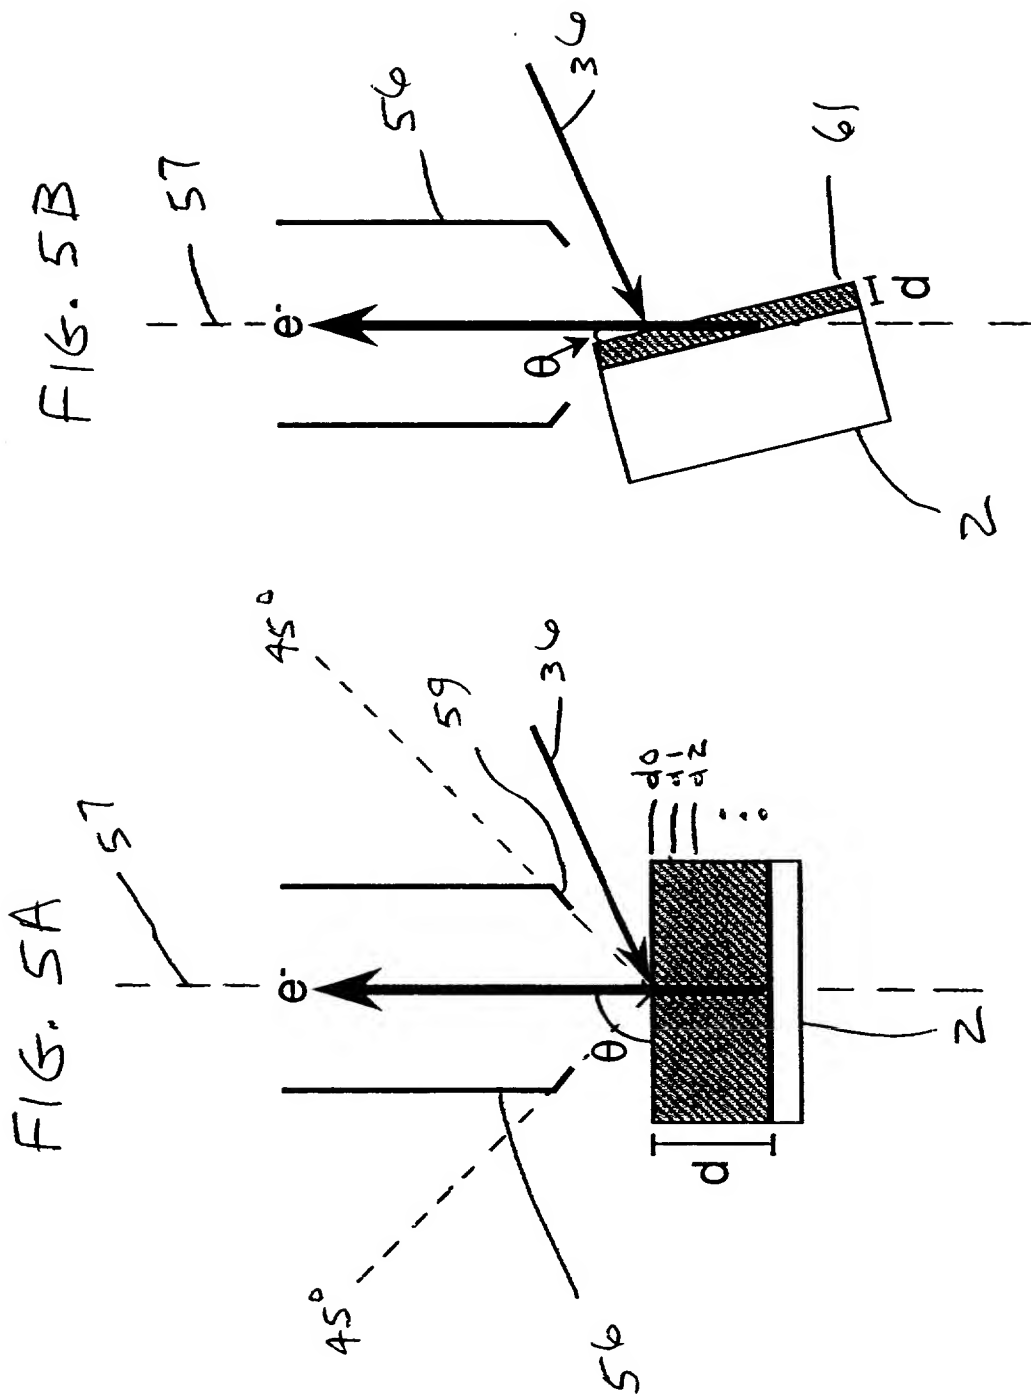


FIG. 6

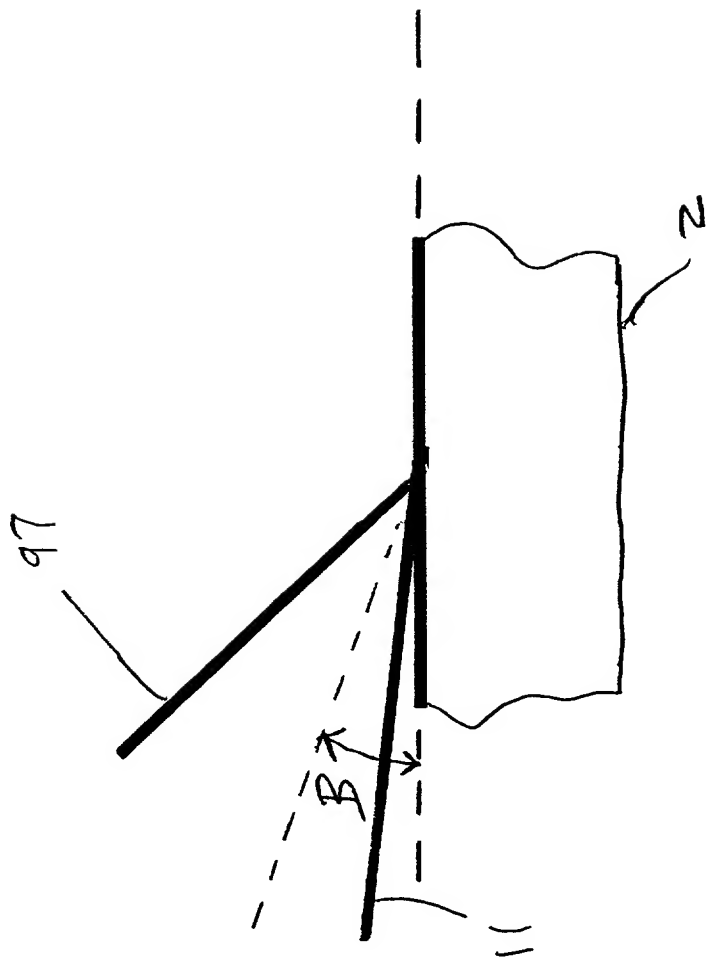


FIG. 7


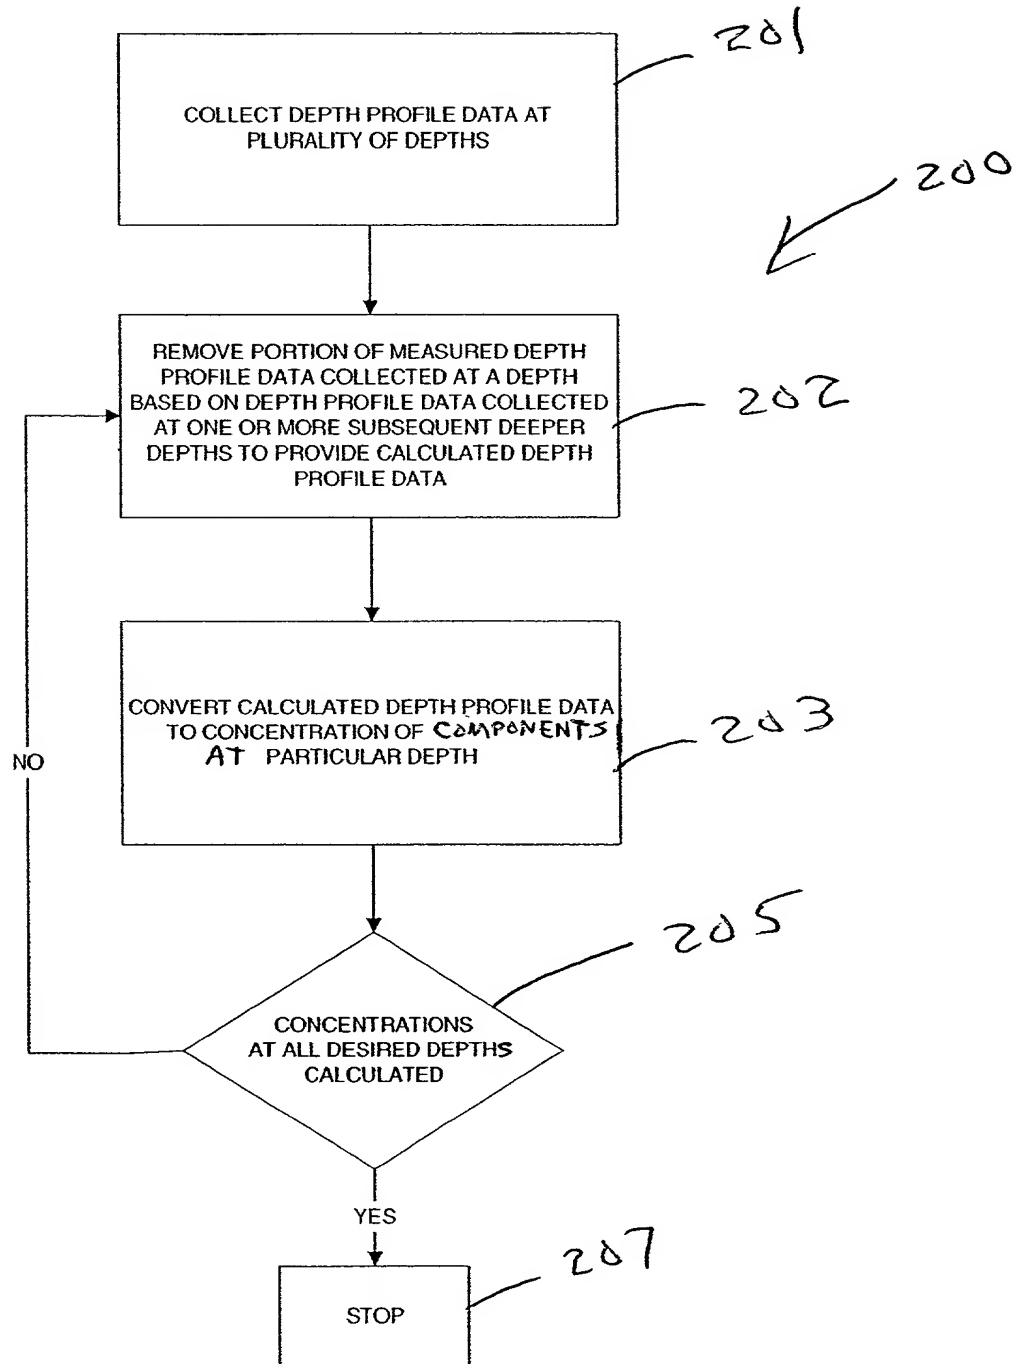


FIG. 7


FIG. 8

230
↓

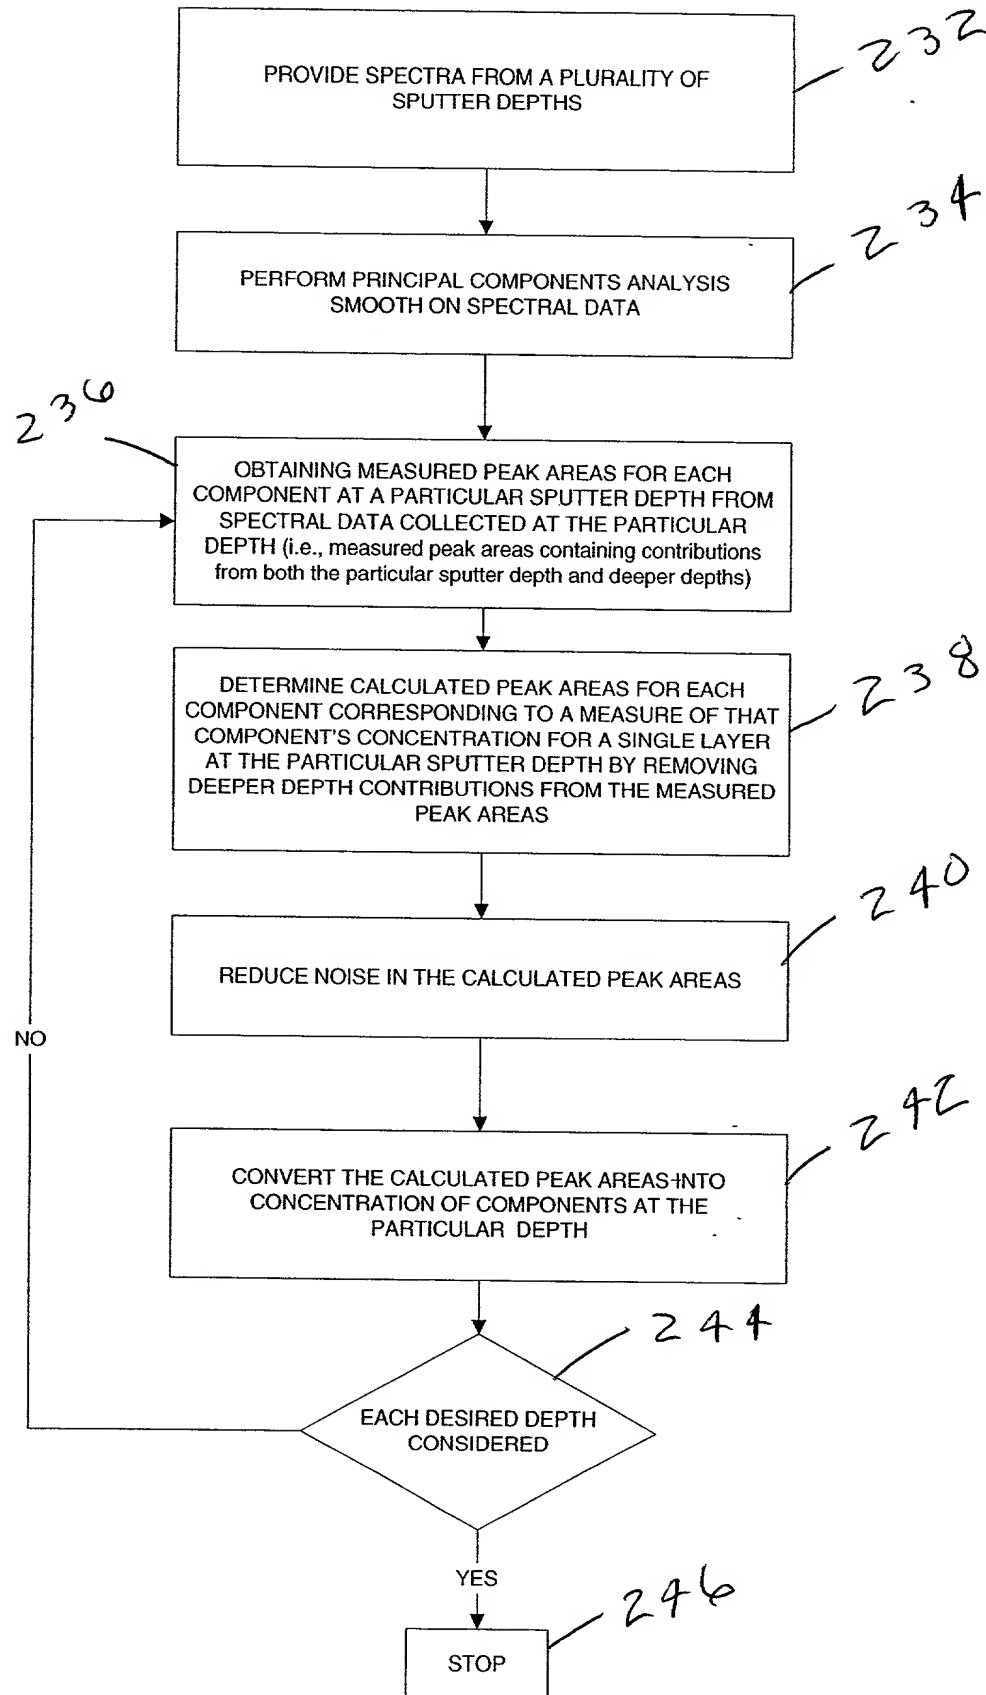

1000344 103604

FIG. 9

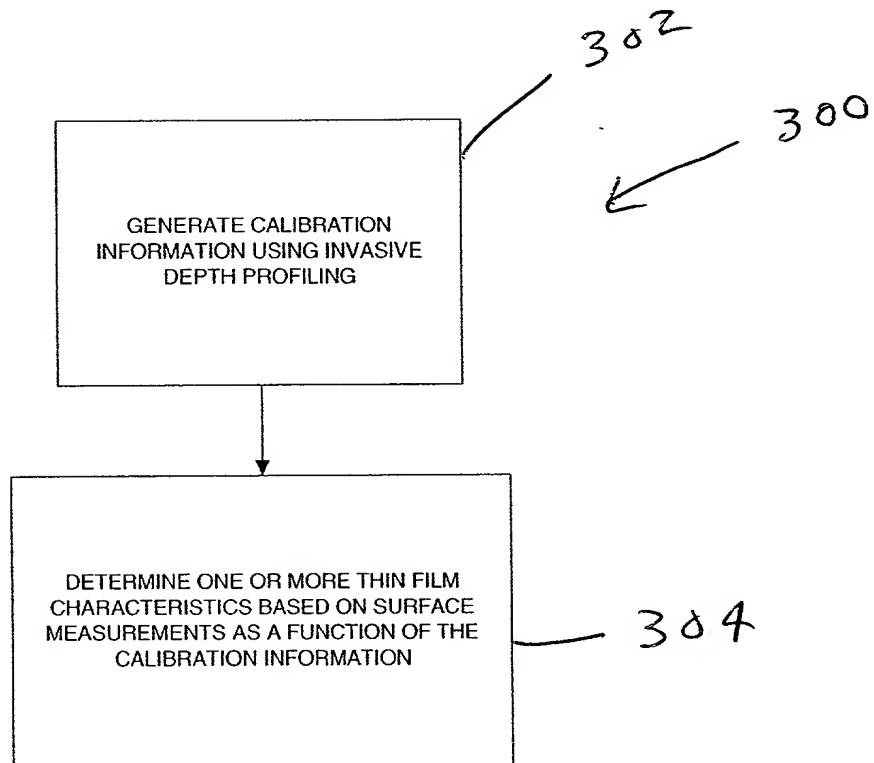

100324-10304

FIG. 10


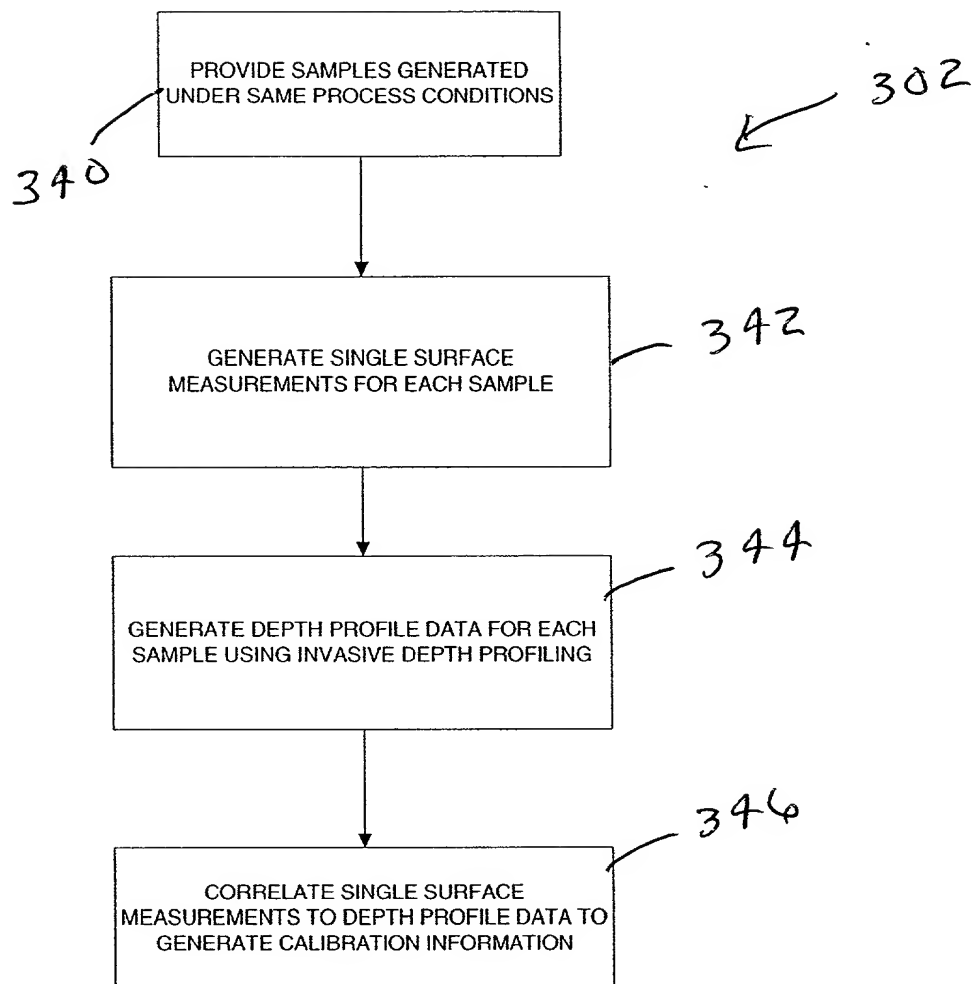


FIG. 10


FIG. 11

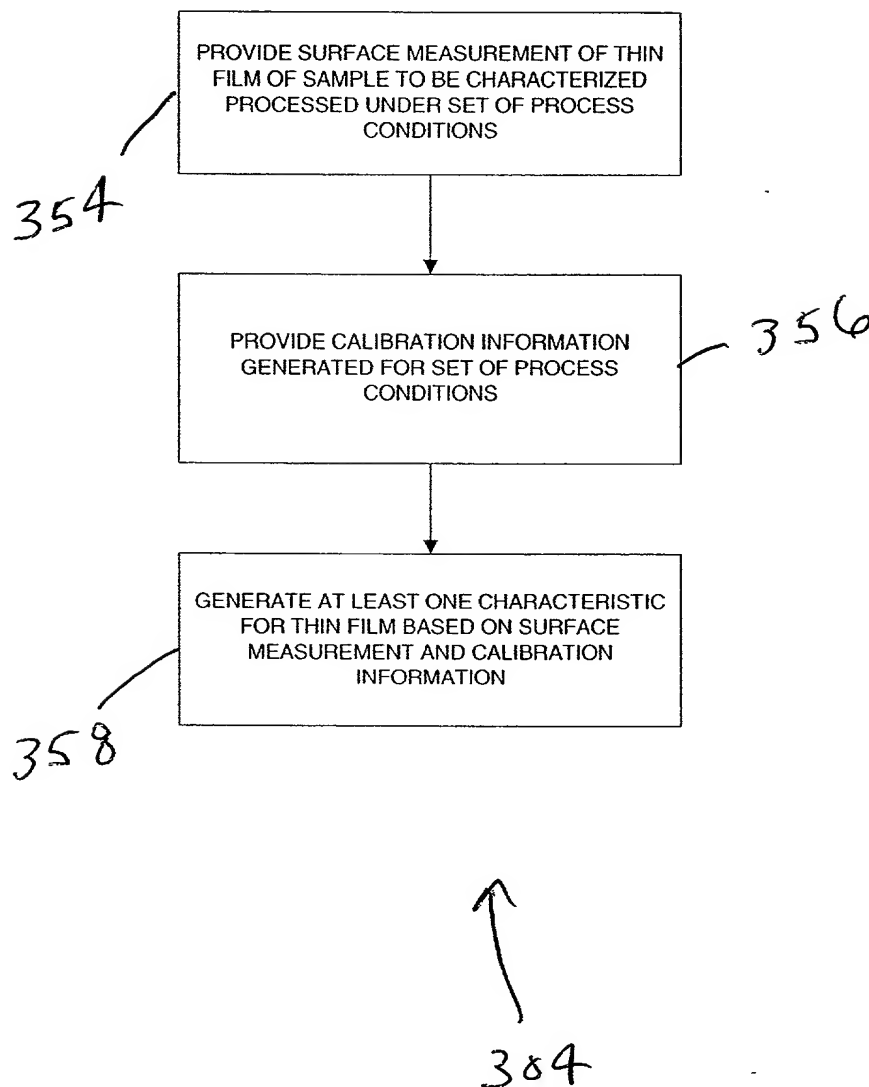

1003224-10301

FIG. 12


(single measurement)

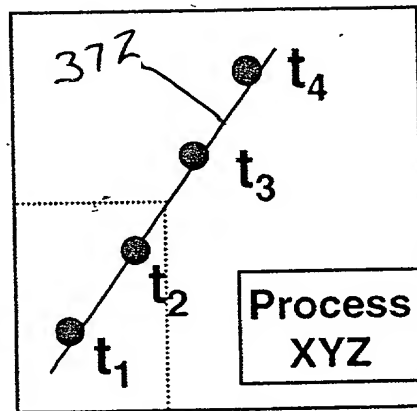

Total N Dose
(calibration with
depth profile)

FIG. 12

FIG. 13

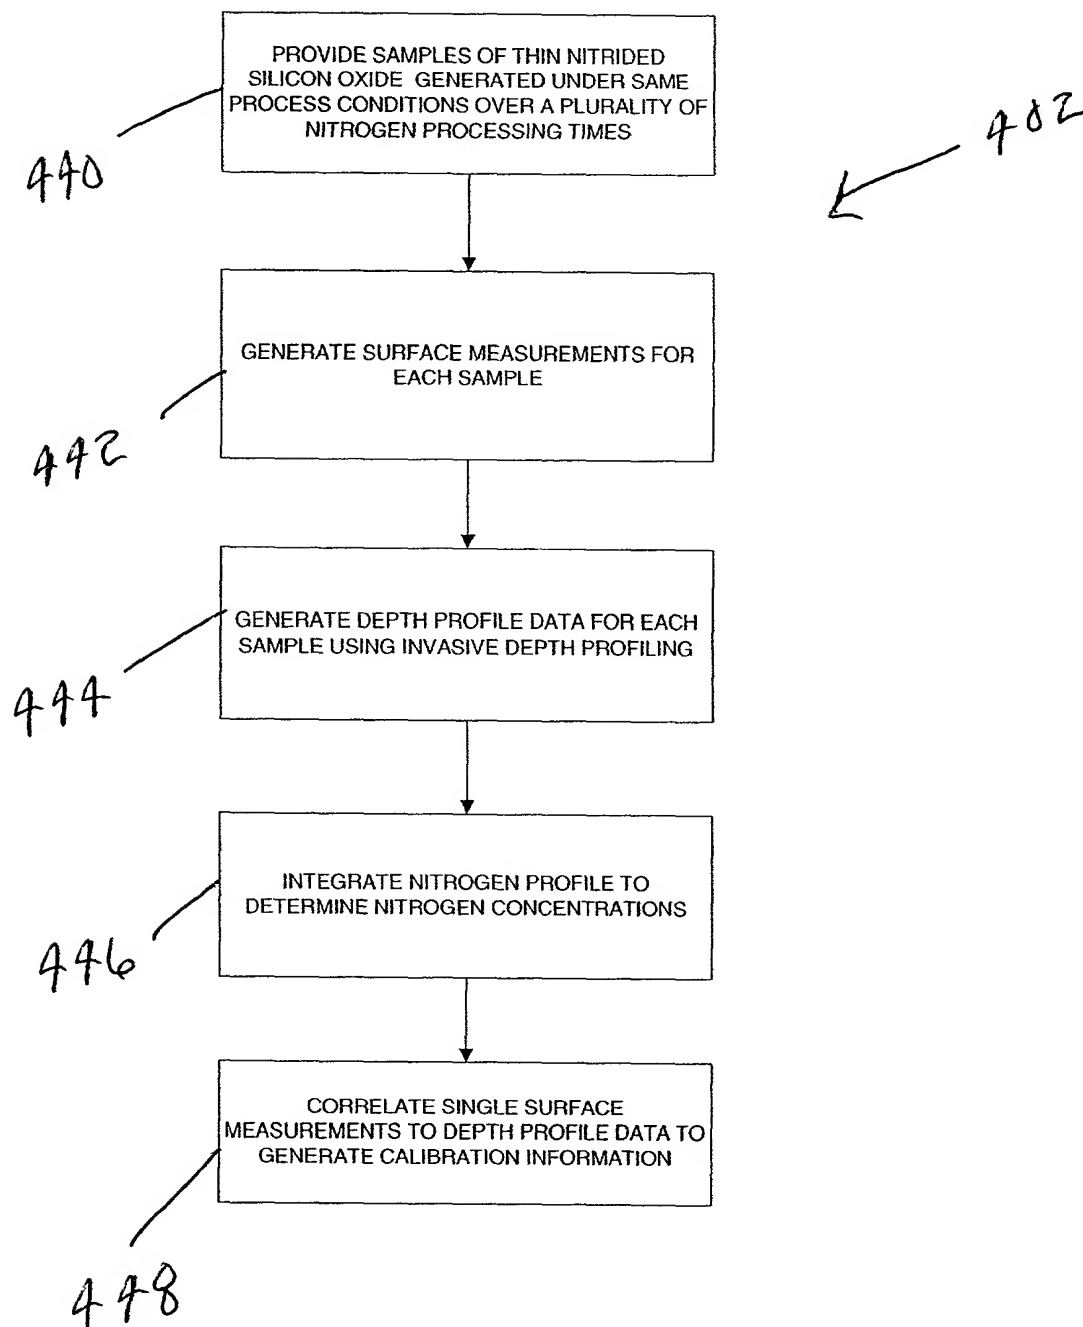

10003224.102601

FIG. 14

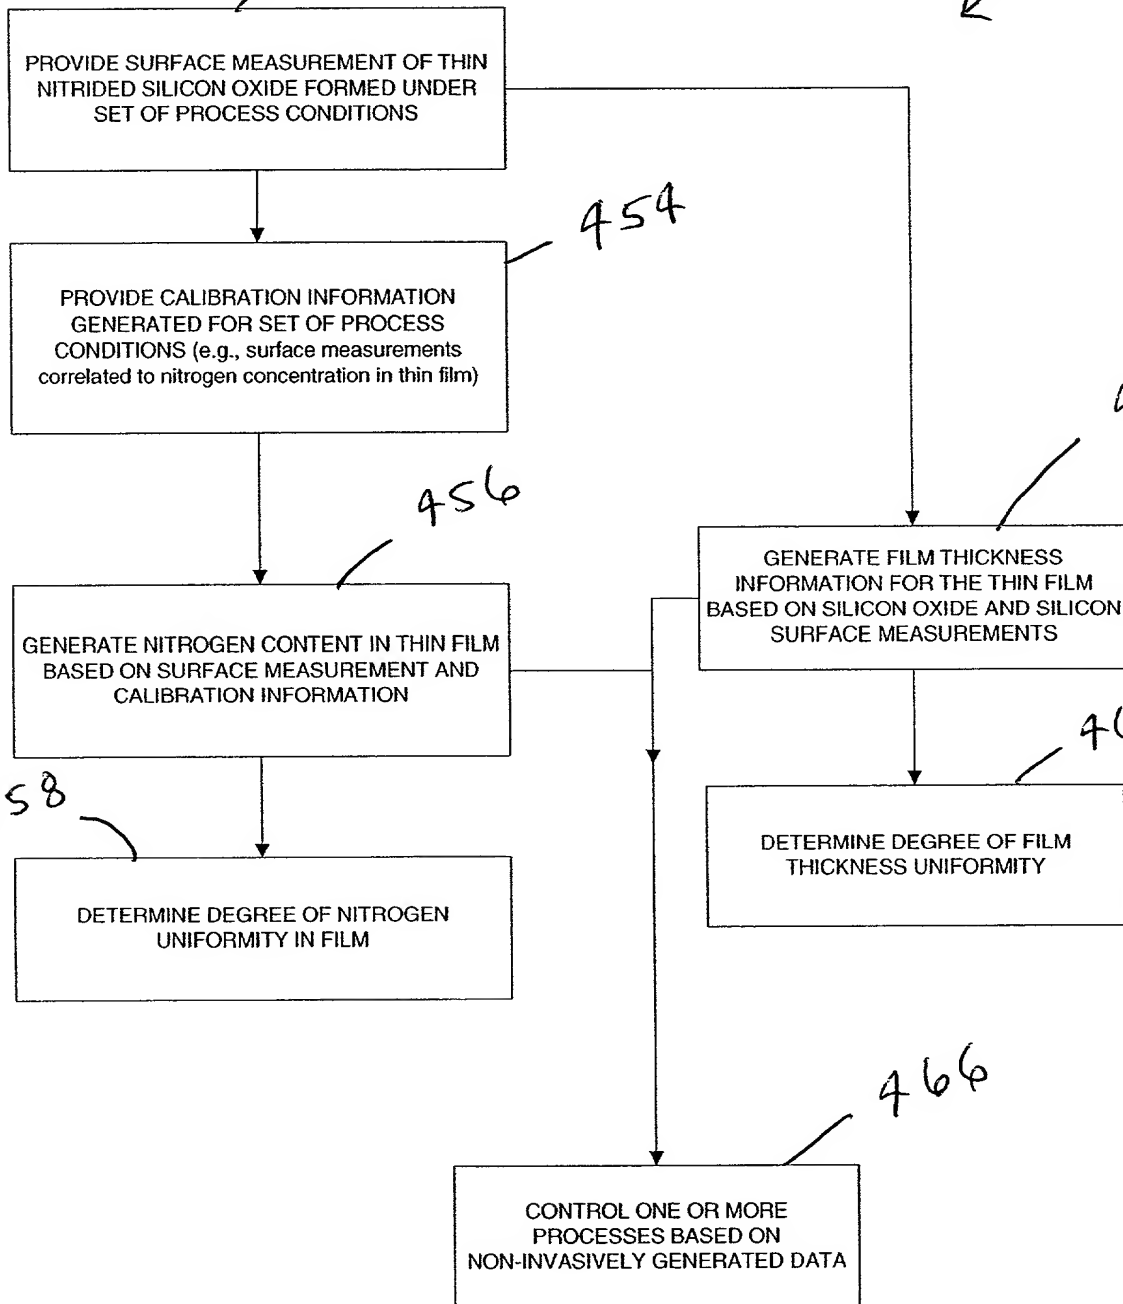


FIG. 15

